


DOCTOR INSTRUCTIONS

Thank you for purchasing the Vision Assessment Corporation Chain Polarized Variable Vectograph Vision Therapy System (P/N 1056).

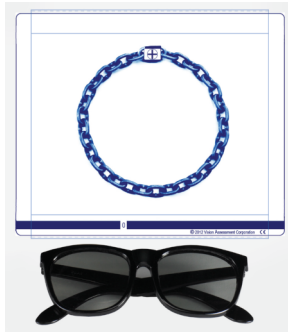

PURPOSE

A three-dimensional picture is used to strengthen the binocularity system and provide base-in and/or base-out training.

FAMILIARIZE YOURSELF WITH THE VECTOGRAPH

- Polarized Variable Vectograph Vision Therapy System consists of:

2. 1 Guide



3. 2 Vectographic Panels

- Panel 1 (Blue Bar at Bottom)



- Panel 2 (Numbers/Letters at Bottom)



4. 1 Pair Standard Polarized Viewers



(NOT TO BE USED AS SUNGLASSES)

5. 2 Instruction Manuals

- Doctor Instruction Manual
- Patient Instruction Manual

This exercise works best if practiced daily as suggested. A Patient Instruction Manual has been included so the Vectograph Vision Therapy System can be sent home with the patient to allow for greater success through continued at-home usage and practice.


6. 1 Patient Vision Therapy Record Form with Pen

TESTING CONDITIONS

- Well-lit, glare-free area
- If reflections or glare on the Vectograph can be seen, try tilting it or choose another testing location.

ADMINISTRATION

1. Place the polarized viewers on the patient.
PLEASE NOTE: DOCTOR SHOULD ADVISE WHETHER OR NOT POLARIZED VIEWERS SHOULD BE WORN OVER PATIENT'S PRESCRIPTION GLASSES.
2. Hold the Vectograph approximately 16 inches (40 cm) in front of the patient.
3. Slide the 2 panels in the guide until the 0 appears in the opening on the blue bar at the bottom of the test.
4. Now ask the patient to look at the Lock on the Chain containing the + at the top of the Chain image.
5. The patient should be able to see a +. If the patient is unable to see a + the patient is suppressing vision in one eye.
 - If the patient only sees the horizontal portion of the cross, the patient is suppressing vision in the Right Eye. Instruct the patient to cover their Left Eye. Have the patient focus with their Right Eye until he/she is able to see the vertical portion of the cross that could not be seen when viewing the Vectograph binocularly. Then again have the patient view the Vectograph binocularly to ensure that both the horizontal and vertical parts of the + can be seen.
 - If the patient only sees the vertical portion of the cross, the patient is suppressing vision in the Left Eye. Instruct the patient to cover their Right Eye. Have the patient focus with their Left Eye until he/she is able to see the horizontal portion of the cross that could not be seen when viewing the Vectograph binocularly. Then again have the patient view the Vectograph binocularly to ensure that both the horizontal and vertical parts of the + can be seen.
6. Once the patient can see the + sign (both the vertical and horizontal portions of the cross), the patient is ready to use the Vectograph.
7. Slowly slide the panels apart and ask the patient to try to maintain a single Chain image. *As the panels are separated and the blue bar moves along the letters from A to P, the Chain image should get larger and float behind the Vectograph (divergence). As the panels are separated and the blue bar moves along the numbers from 1 – 24, the Chain image should get smaller and float in front of the Vectograph (convergence), also known as the SILO Effect "Small In, Large Out."*
8. Have the patient notify you when he/she is no longer able to fuse the Chain image, or when the Chain image doubles. (This is the Breaking Point.)
9. Note the number/letter in the space on the blue bar at the bottom of the Vectograph. Refer to "Scoring" section of this manual.
10. Next, as you slowly slide the panels back together, ask the patient to notify you when he/she is able to see the Chain image as a single clear image again. (This is the Recovery Point.)
11. Note the number/letter in the in the space on the blue bar at the bottom of the Vectograph. Refer to "Scoring" section of this manual.
12. The Chain floats out slightly at the bottom of the image so as to appear that the patient can loop an object with the Chain. Place a small object on a table in front of the patient. Hold the Vectograph so that the patient

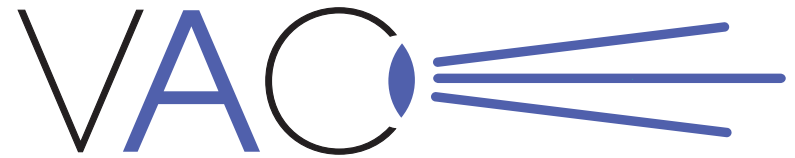

Vision
Assessment
Corporation™

Chain

Polarized Variable Vectograph

P/N 1056
DOCTOR INSTRUCTIONS

Vision Assessment Corporation
5400 Newport Drive, Suite 3
Rolling Meadows, Illinois 60008 USA
Phone: 1 847 239 5889
Email: [sales @VisionAssessment.com](mailto:sales@VisionAssessment.com)
Web: www.VisionAssessment.com


can view the object on the table in the center of the Chain image. Slowly slide the panels apart and ask the patient to focus on the object in the center while trying to maintain a single fused image.

- Repeat steps 7 –11 using the object as described in step 12.
- Repeat steps 7 – 11 until patient can achieve the doctor's recommended goal.

SCORING

- Each letter on the bottom blue bar represents one diopter. (Base-In) (Divergence / Relaxing)
- Each number 1-10 on the bottom blue bar represents one diopter. (Base-Out) (Convergence / Crossing)
- Each number 10-24 represents two diopters. (Base-Out) (Convergence / Crossing)
- 40 diopter range of separation available.
- Refer to the Patient Vision Therapy Record Form.
- Record the date.
- Above the diagonal line in the row labeled "Relaxing" record the Breaking Point for the highest letter that the patient is able to reach.
- In the same box below the diagonal line record the Recovery Point for the highest letter at which the patient is able to fuse the images as a single clear image again.
- Repeat the previous 2 steps for the row labeled "Crossing" for recording the Breaking Point and Recovery Point for the highest numbers that the patient can reach on the blue bar at the bottom of the Vectograph.

CARE/HANDLING & STORAGE

- Clean vectographic panels and guide with a soft, damp, lint-free cloth. Dampen cloth using glass cleaner or mild detergent/water.
- CAUTION: DO NOT IMMERSE THE VECTOGRAPHIC PANELS IN WATER. DO NOT SPRAY CLEANER DIRECTLY ONTO PANELS.**
-  Store Vectograph in a dry place away from direct sunlight.
- Clean polarized viewers using lens cleaner and soft, lint-free cloth.
- If panels are removed from guide during cleaning, replace the panels in the guide placing the panel with the blue bar on top of the panel with the numbers/letters and ensuring that the plastic portion of the guide is behind the panels.

WARRANTY

- 1 year manufacturer warranty from date of purchase.

Notice to User/Patient: *Any serious incident that has occurred in relation to this device should be reported to the manufacturer and to the competent authority of the Member State in which the user and/or patient is established.*



MDSS GmbH,
Schiffgraben 41, Hannover 30175, Germany